

# Wobble-not™

## Low Insertion Force Serological Pipet

patent pending


**Unique NO DRIP design**

**See the Difference. Feel the Difference.**

### Standard Pipet

If you don't use enough force, the plug end is not held tightly and the pipet is wobbly.

To get the pipet to wobble less, you must use much more force to insert it.

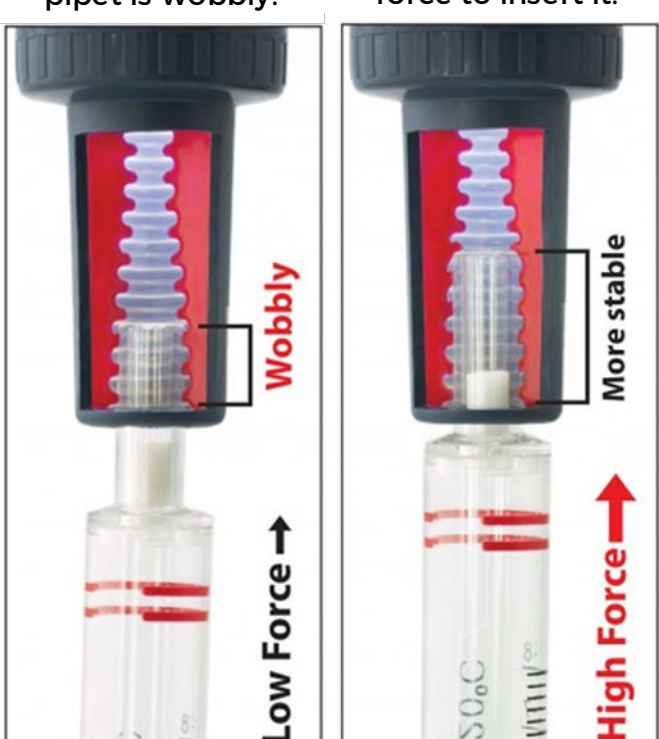

### Wobble-not™


With low insertion force, the Wobble-not pipet is held stably.

All pipet controllers have the same basic nozzle design for holding onto serological pipets.



**Low insertion force = Less wrist strain = Less pain = More ERGONOMIC!**



## Why it Works

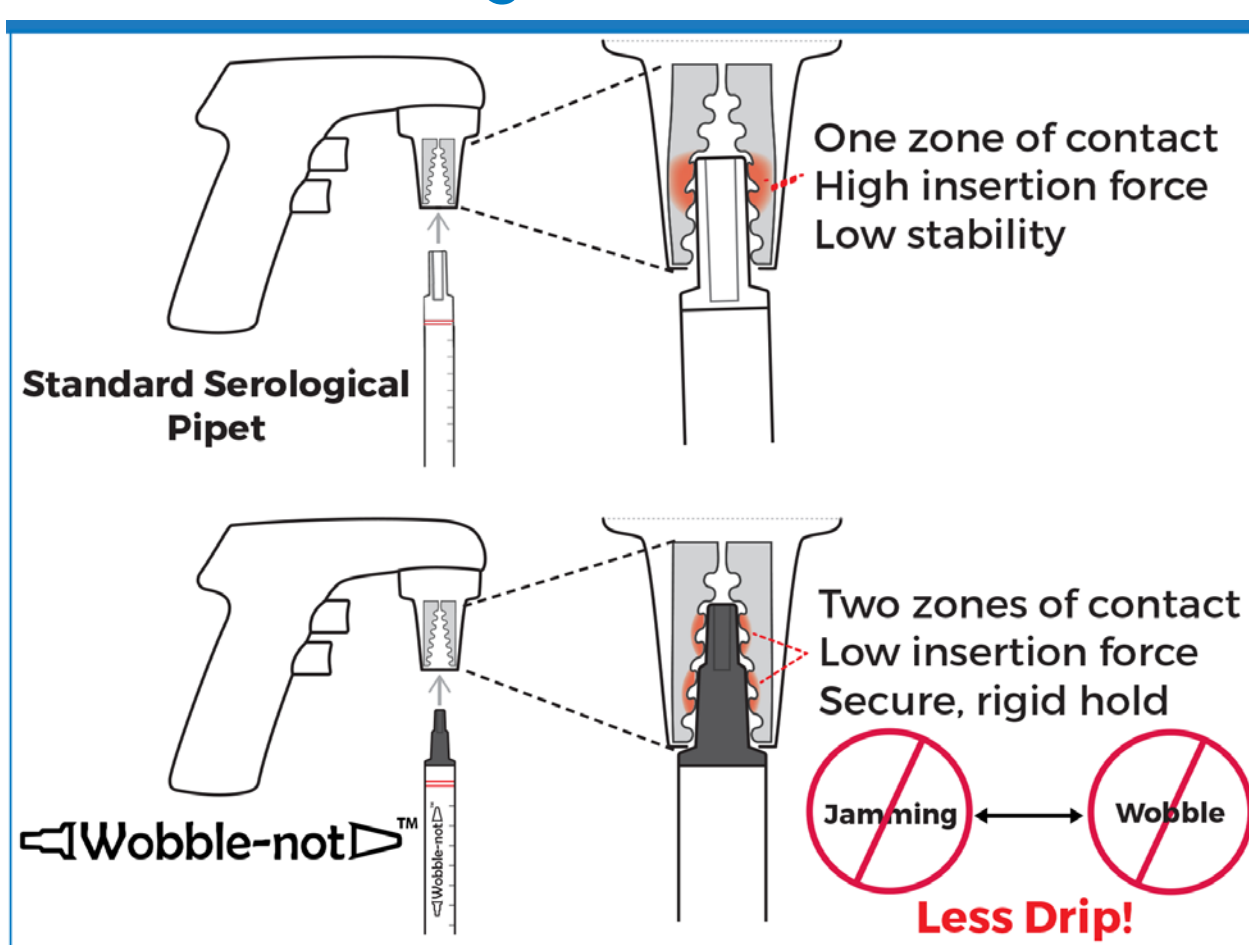

**Less Sag = Less Wobble = Less Drip!**


### Standard Serological Pipet

### Wobble-not™

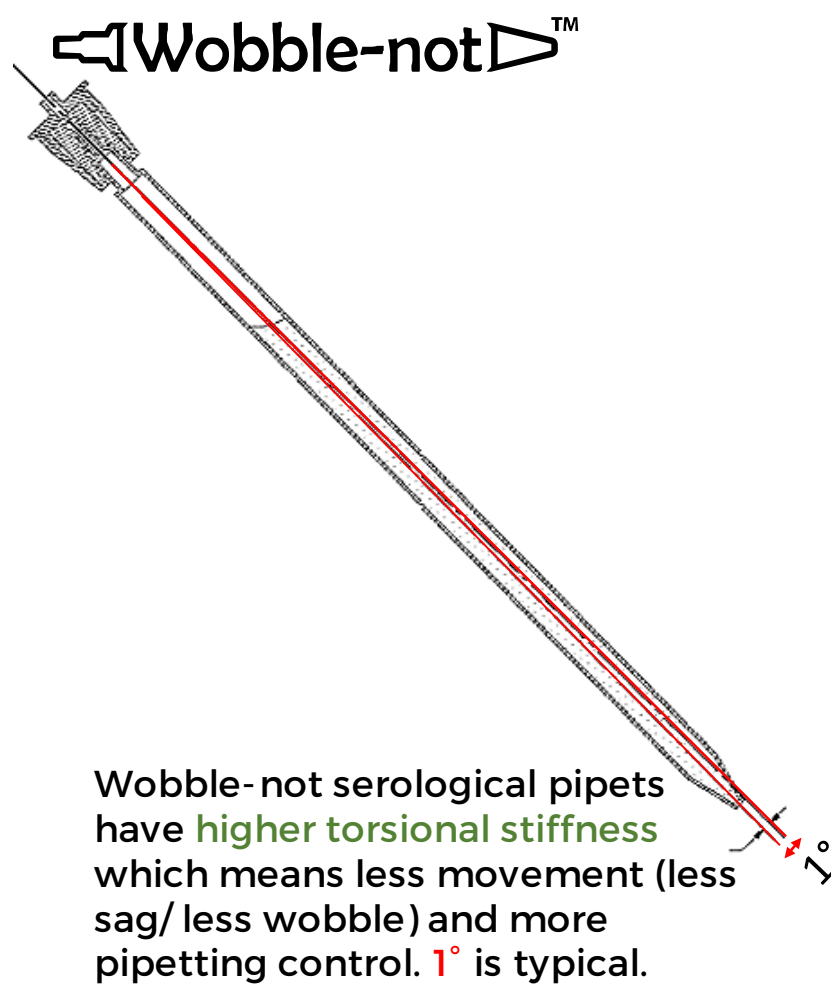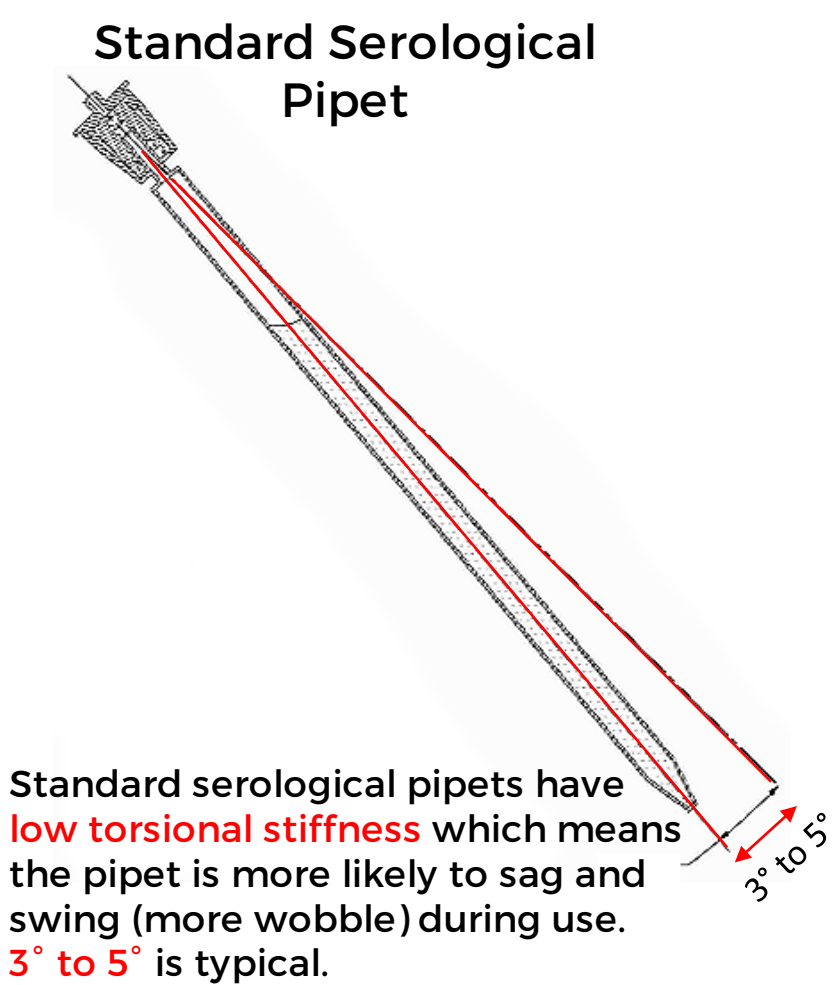

## Wobble-not Makes a Difference Ergonomically and Practically!


**Achieve Minimal Wobble at Low Force with Wobble-not**

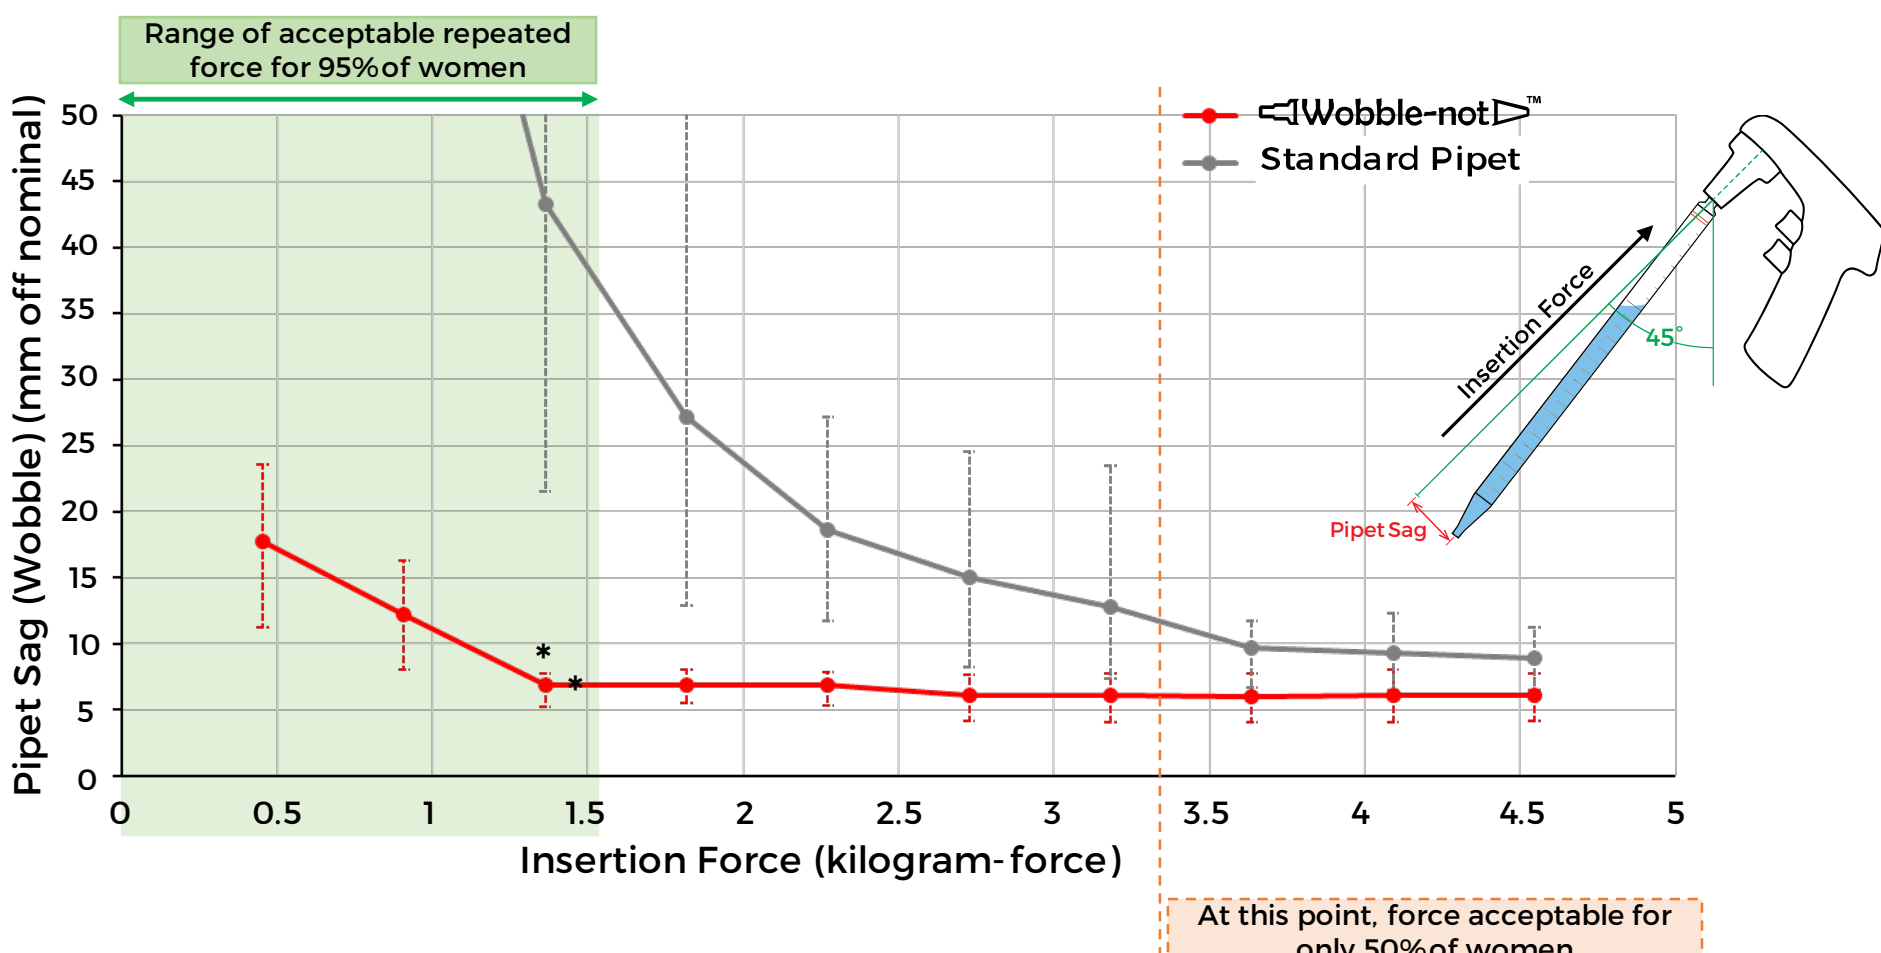

The amount of sag (wobble) from a nominal pipetting angle was measured at each kilogram-force of insertion into a typical pipette controller. With Wobble-not serological pipets, minimal pipet sag (wobble)\* was achieved with a pipet insertion force of 1.4 kilogram-force which is well within the range of acceptable repeated force for 95% of women. At this same kilogram-force, standard serological pipets have more than 5X sag (wobble) and never reach the minimal wobble levels of the Wobble-not.

## Try Wobble-not with Your Favorite Pipet Controller!

**Less Insertion Force & Less Wobble with Wobble-not**

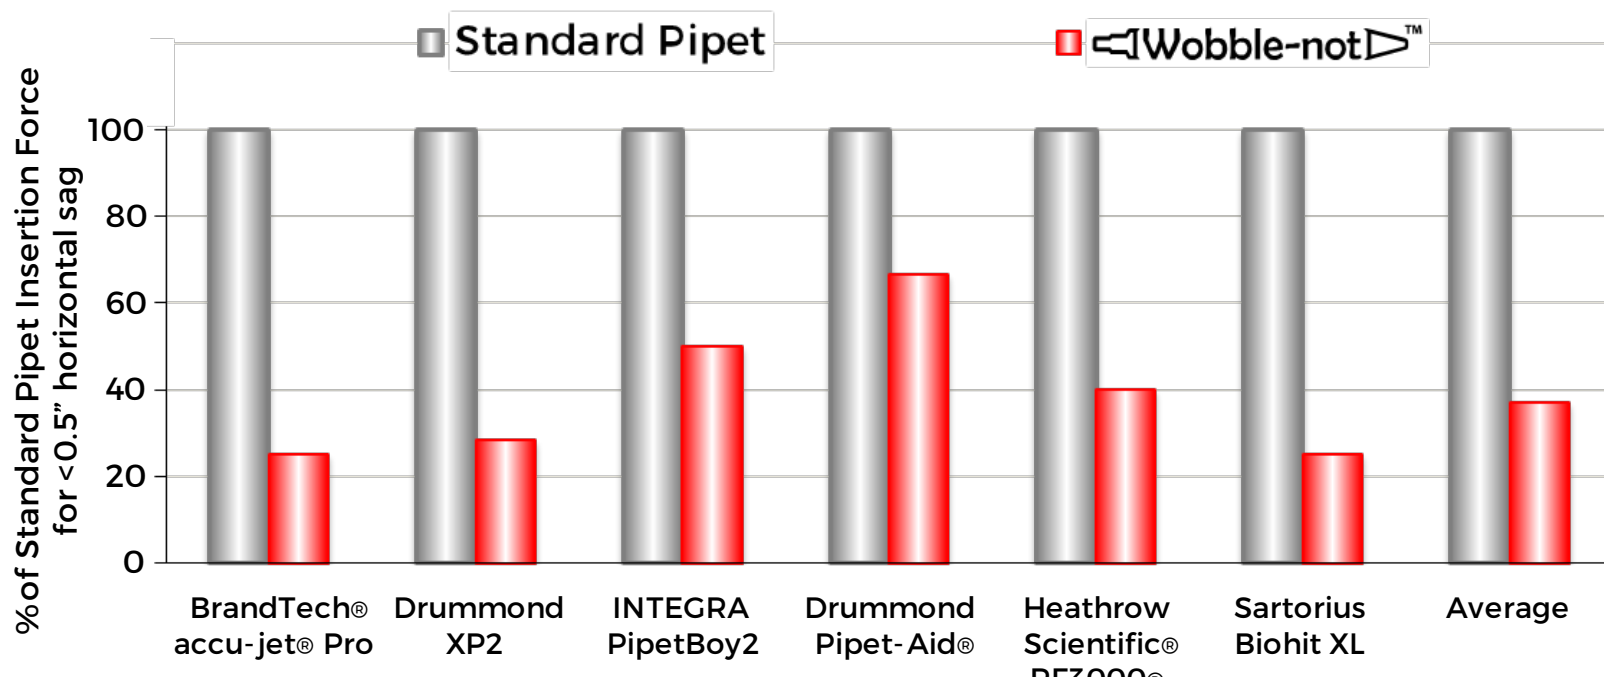

The insertion force needed to achieve sag (wobble) of 0.5 inches or less from horizontal was determined using Standard Pipet and Wobble-not serological pipets with a variety of pipette controllers. The force for the Standard Pipet using each controller was set at 100% and relative %force with Wobble-not determined. With every controller tested, Wobble-not pipets required less force for the low level of pipet wobble.